


Thermo Scientific Synchronis C18 HPLC Columns

Consistent, predictable separations,
Column after column, time after time

- Outstanding reproducibility
- Highly pure, high surface area silica
- High carbon load for increased retention
- Double endcapped for extra surface coverage
- Highly inert towards basic compounds
- Rigorously tested to ensure quality

Specifications

Particle size	1.7 μm , 3 μm , 5 μm	Carbon load	16 %
Pore size	100 \AA	Endcapped	Yes
Surface area	320 m^2/g	USP classification	L1
pH range	2-9		

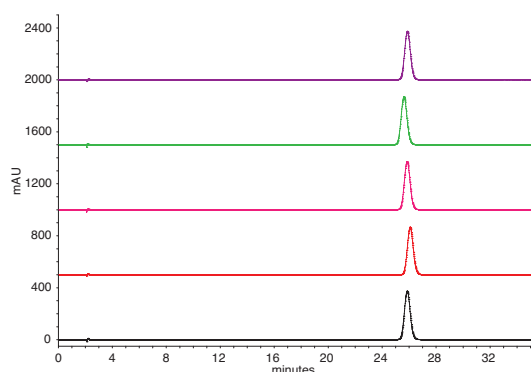

Column	Retention Time (min)	Efficiency	Peak Area
1	25.82	62069	11532105
2	26.03	61688	11543904
3	25.90	62657	11527718
4	25.66	61317	11463444
5	25.92	63142	11520618
Inter-column precision (% RSD)	0.52	1.18	0.27



Outstanding column to column reproducibility

When developing a new method, one of the most important goals for the chromatographer is to achieve a consistent, reproducible separation. The selection of a highly reproducible HPLC column is essential if this goal is to be attained.

Thermo Scientific™ Synchronis™ C18 HPLC columns show excellent column to column reproducibility, as illustrated here by the analysis of zidovudine using five separate columns.

The reproducibility in terms of retention time and peak area is less than or equal to 0.5%, column to column. This indicates that the columns are well packed.

The variation in peak area is 0.27%, which is important for quantitation of analytes.

Synchronis C18 HPLC columns achieve this goal, starting from the highly pure, high surface area silica and dense bonding, all controlled and characterized through the use of rigorous testing.

New, enhanced, automated column packing methods drive consistency even further and every column is individually tested to ensure that it meets the required specifications. These extensive testing and quality control procedures ensure the delivery of a consistent product, column after column.


Column:
Mobile phase:
Flow rate:
Temperature:
Detection:
Injection volume:

Synchronis C18 5 μm , 250 mm x 4.0 mm
water:methanol (4:1)
1.0 mL min^{-1}
25 $^{\circ}\text{C}$
265 nm
10 μL

1. Zidovudine

Thermo
SCIENTIFIC

Application: Chloramphenicol (USP)

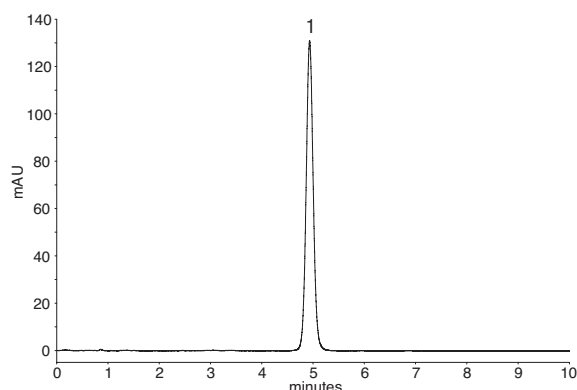

Column: Synchronis C18 5 µm, 100 mm x 4.6 mm
Mobile phase: water:methanol:glacial acetic acid (54.9:45:0.1)
Flow rate: 1.0 mL/min
Temperature: 25 °C
Detection: 280 nm
Injection volume: 10 µL

1. Chloramphenicol

Parameter	USP Specification	Measured (6 replicate injections)
Efficiency (N)	> 1800	6164
Tailing factor	< 2	1.06
%RSD retention time	< 1%	0.03%
%RSD peak area	< 1%	0.32%

Ordering Information

Description	Particle Size	Length (mm)	2.1 mm ID	3.0 mm ID	4.0 mm ID	4.6 mm ID
Synchronis C18	1.7 µm	30	97102-032130	–	–	–
		50	97102-052130	97102-053030	–	97102-054630
		100	97102-102130	97102-103030	–	–
	3 µm	30	97103-032130	–	–	–
		50	97103-052130	97103-053030	–	97103-054630
		100	97103-102130	97103-103030	–	97103-104630
		150	97103-152130	–	–	97103-154630
	5 µm	30	97105-032130	97105-033030	97105-034030	97105-034630
		50	97105-052130	97105-053030	97105-054030	97105-054630
100		97105-102130	97105-103030	97105-104030	97105-104630	
150		97105-152130	97105-153030	97105-154030	97105-154630	
250		97105-252130	97105-253030	97105-254030	97105-254630	
Drop-in guard cartridges (4/pk)	5 µm	10	97105-012101	97105-013001	97105-014001	–
UNIGUARD Guard Cartridge Holder			852-00	852-00	850-00	–

Consistent, predictable separations: Column after column, time after time

Synchronis HPLC columns are manufactured, packed and tested in ISO 9001:2008 accredited facilities. Each lot of silica is tested for the physical properties of the silica support and only released for production if it meets the stringent test specifications.

Each bonded lot of chromatographic packing material is rigorously tested for primary and secondary interactions with the bonded phase.

New, enhanced, automated packing methods drive consistency even further and every column is individually tested to ensure that it meets the required quality.

These extensive testing and quality control procedures ensure the delivery of a consistent product, column after column.

thermoscientific.com/Synchronis

© 2012 Thermo Fisher Scientific Inc. All rights reserved. All trademarks are the property of Thermo Fisher Scientific Inc. and its subsidiaries. Specifications, terms and pricing are subject to change. Not all products are available in all countries. Please consult your local sales representative for details.

USA and Canada +1 800 332 3331
France +33 (0)1 60 92 48 34
Germany +49 (0) 2423 9431 20 or 21
United Kingdom +44 (0)1928 534110
Japan +81 3 5826 1615

China +86 21 68654588 +86 10 84193588
+86 20 83145199 800 810 5118
India +91 22 6742 9494 +91 27 1766 2352
Australia 1 300 735 292 (free call domestic)
New Zealand 0800 933 966 (free call domestic)
All Other Enquiries +44 (0) 1928 534 050

Technical Support
North America +1 800 332 3331
Outside North America +44 (0) 1928 534 440

PS20601_E 09/12S

INTERCHEMISTRY
thermo
scientific
Representante Autorizado

Thermo
SCIENTIFIC
Part of Thermo Fisher Scientific